

20

PRINTER/DISPLAY

PROCESSING UNIT

18

CO₂

16

FLOW

22

PATIENT WYE

12

14

10

PATIENT

Fig. 1

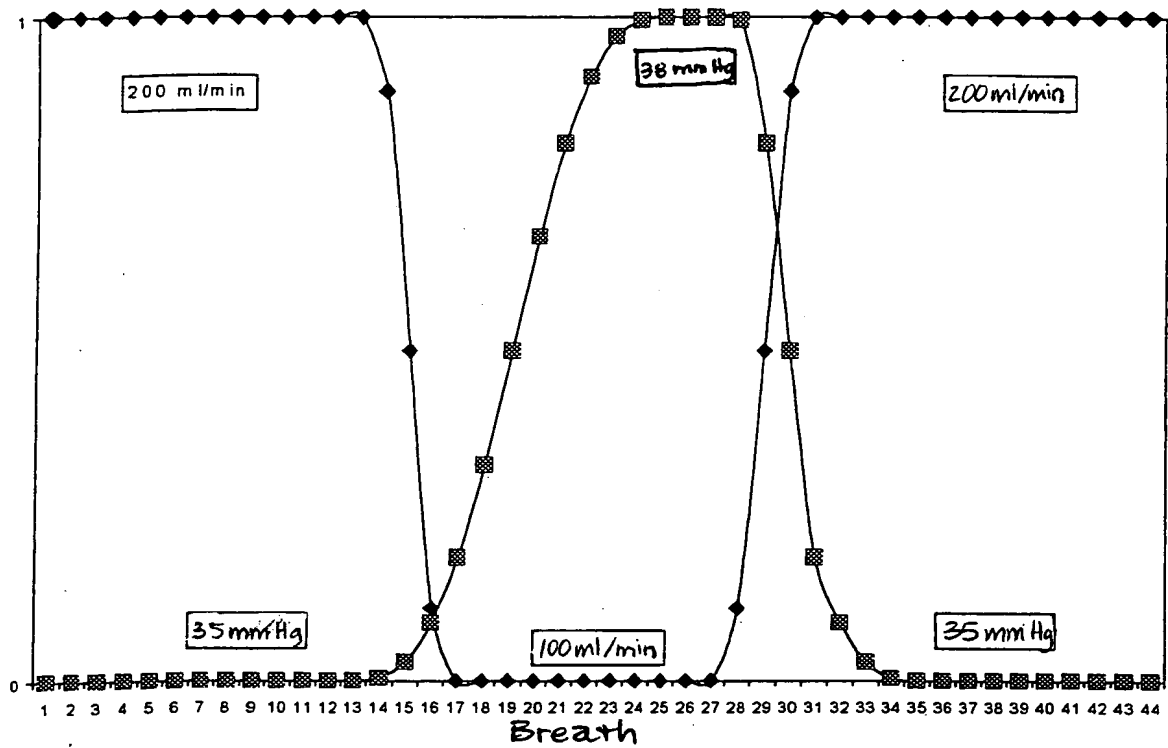


FIG. 2A

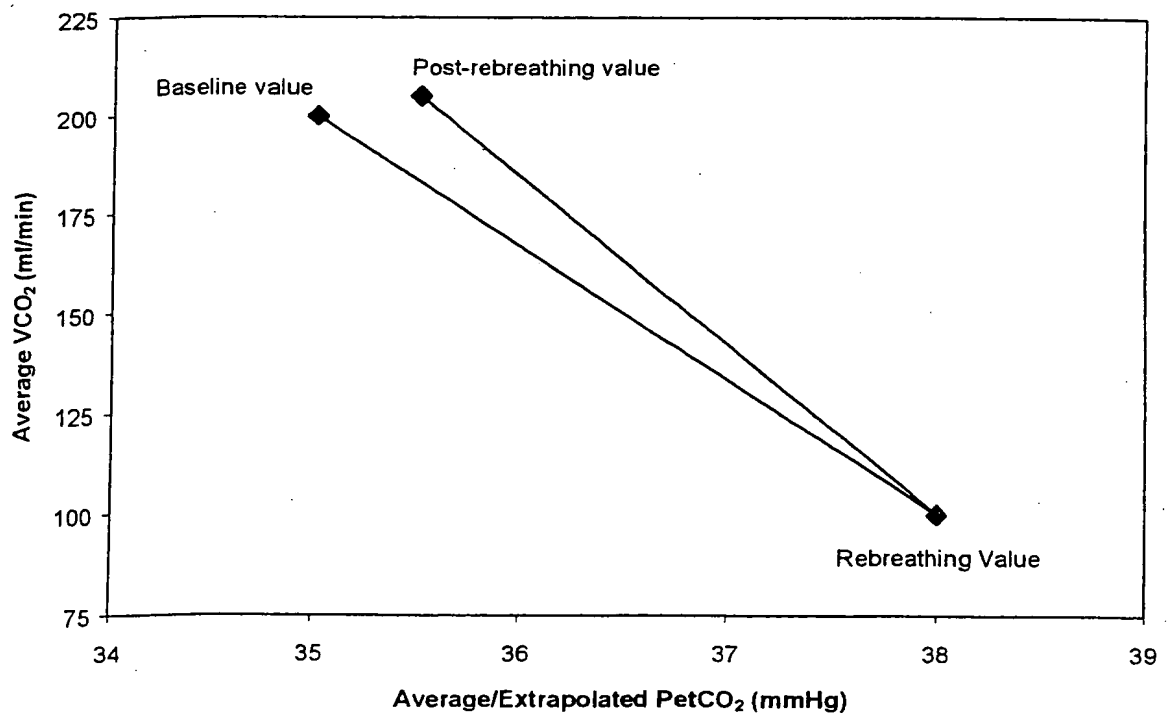


FIG. 2B

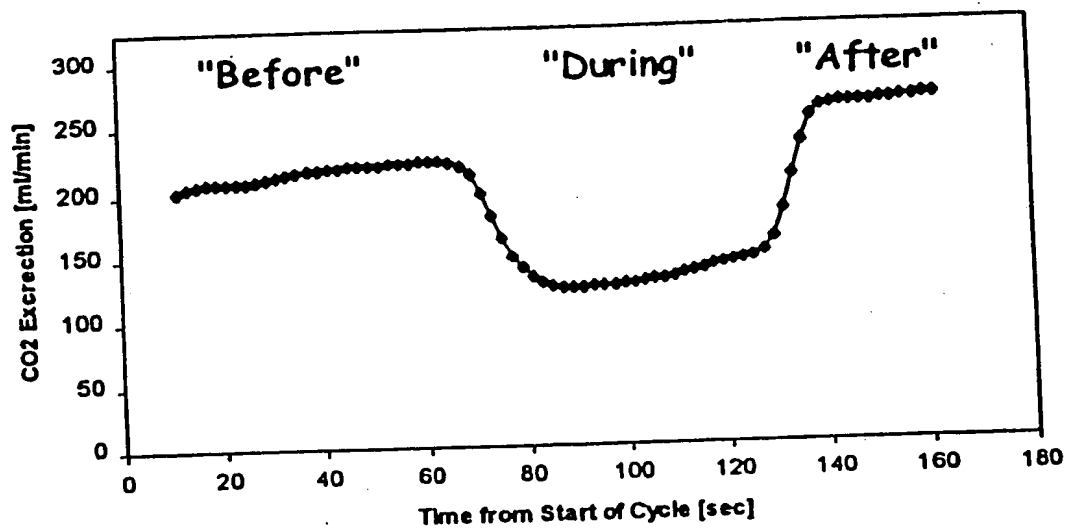


FIG. 3

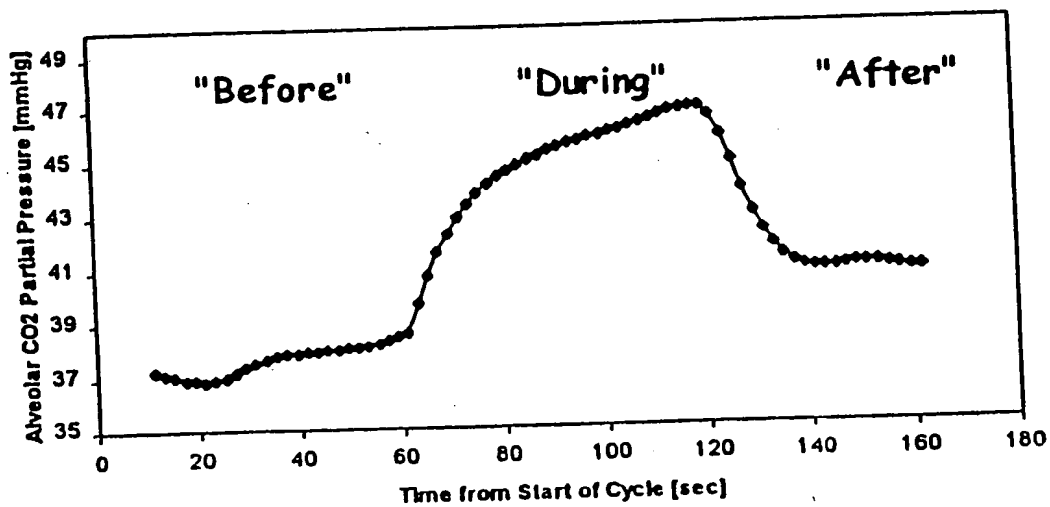


FIG. 4

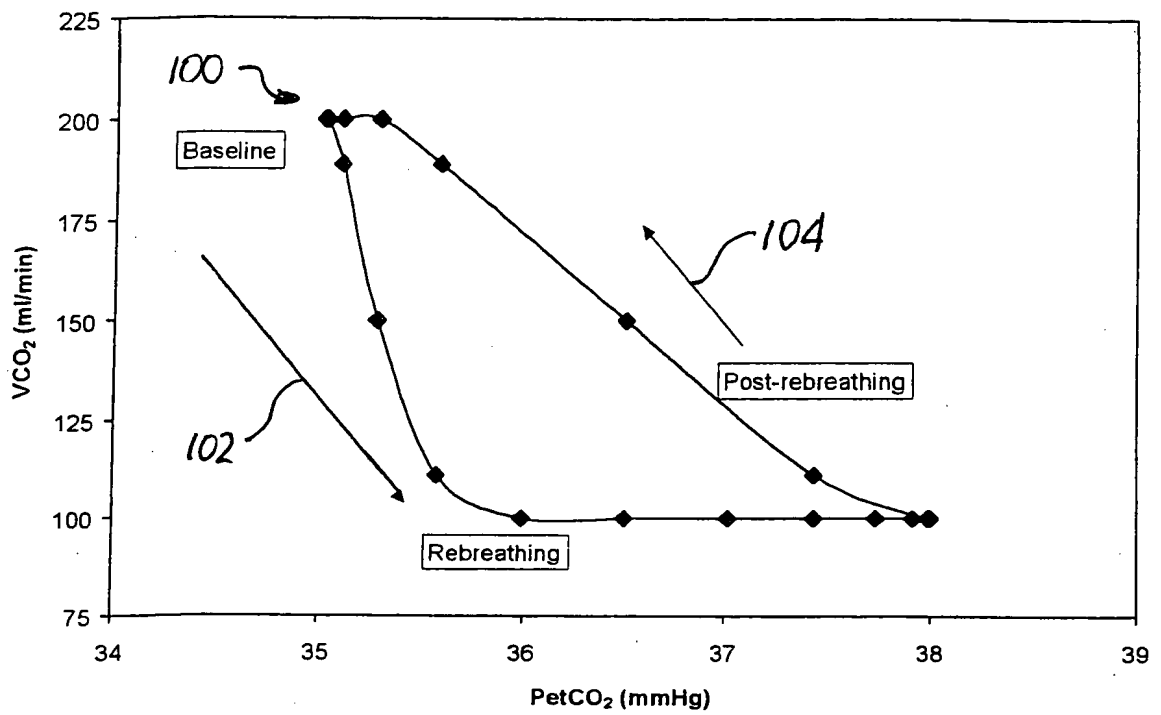


FIG. 5A

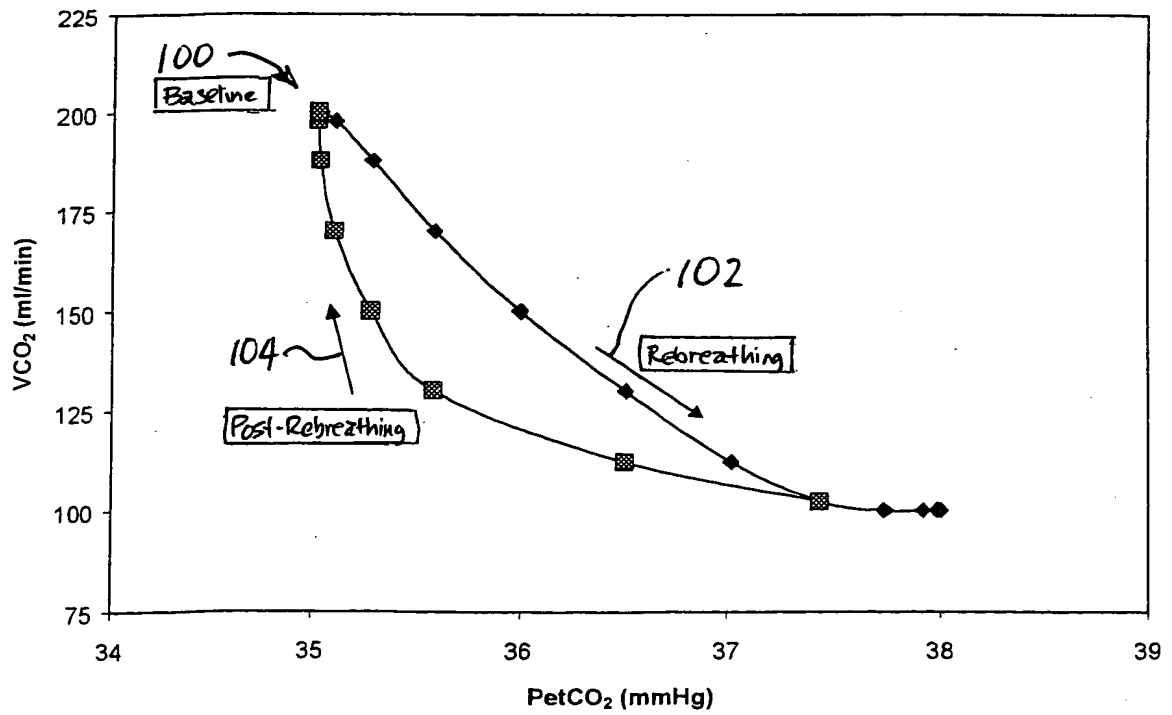


FIG. 5B

100220 5222 F860

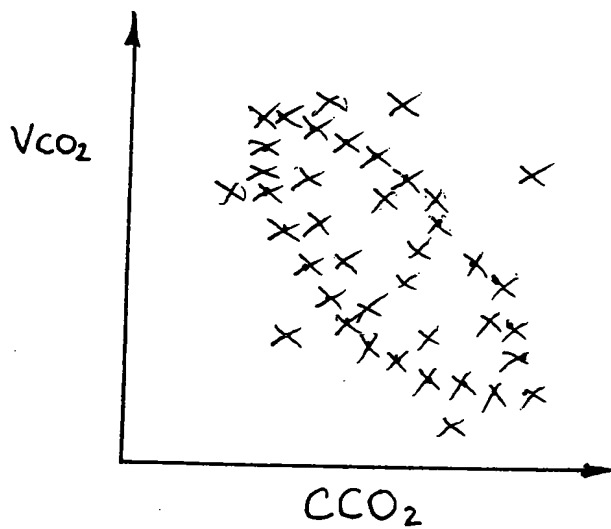


FIG. 6

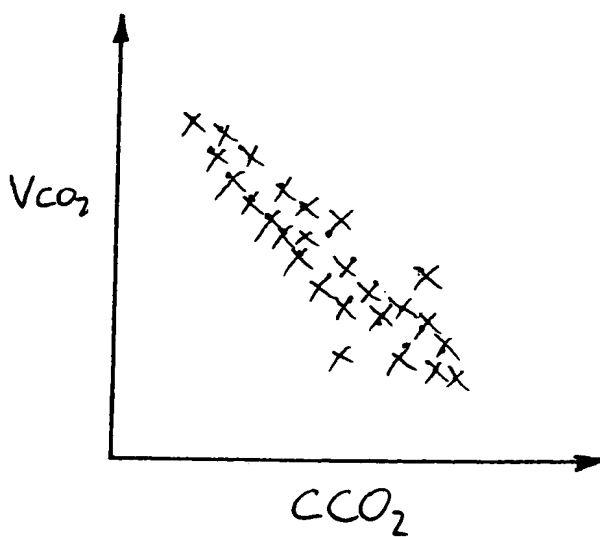


FIG. 7

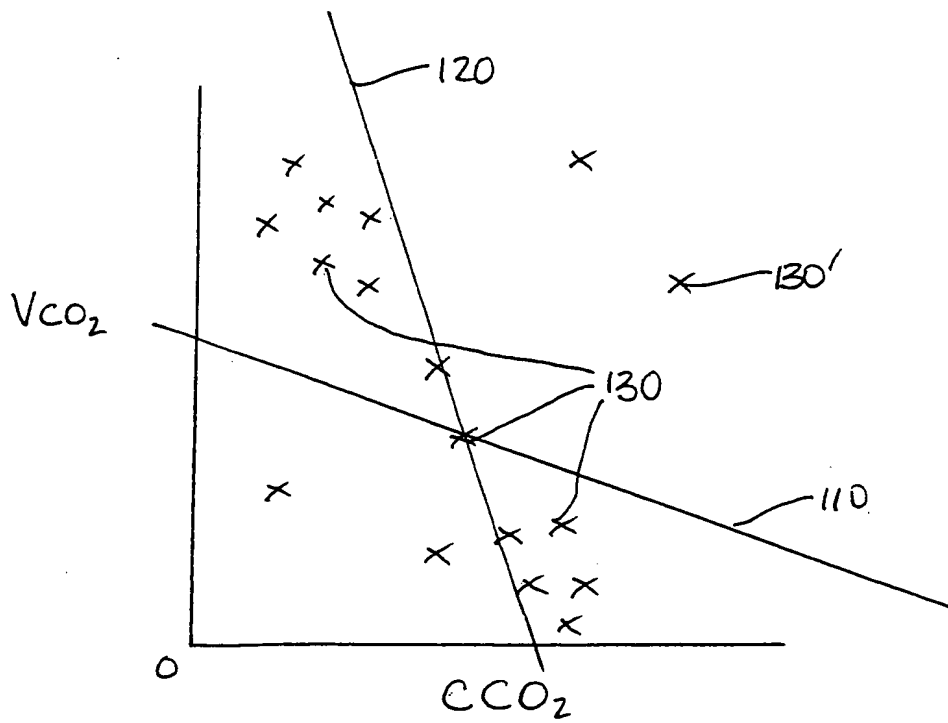


FIG. 8A

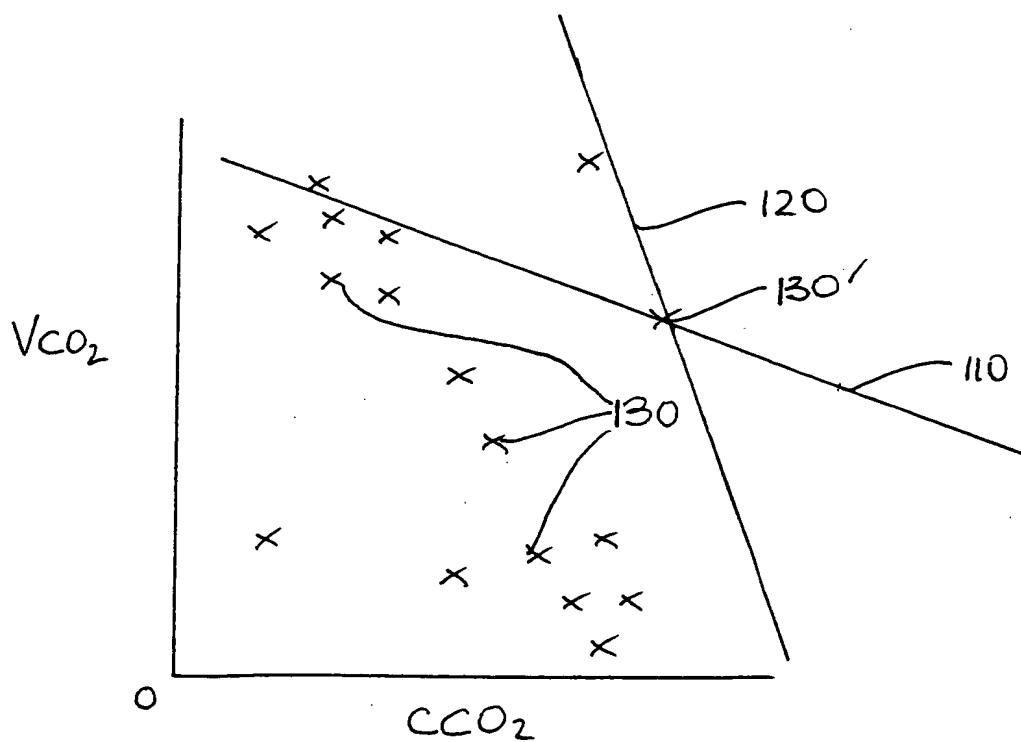


FIG. 8B

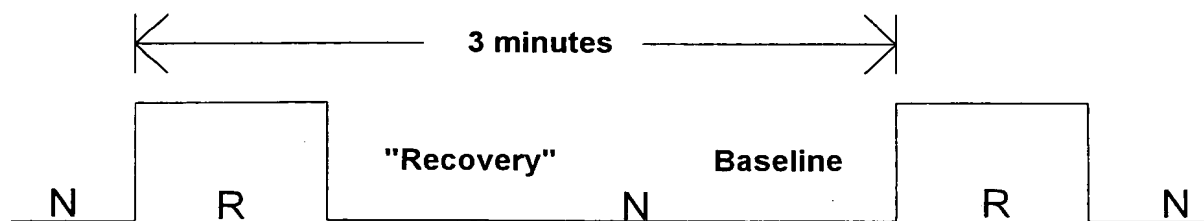


FIG. 9A

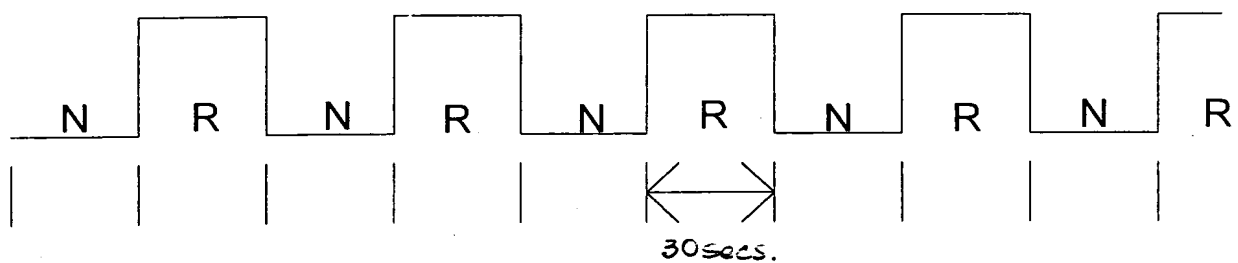


FIG. 9B